

IMPLANT WITH PRESSURE SENSOR FOR GLAUCOMA TREATMENT

Morteza Gharib, et al.

Appl. No.: Unknown Atty Docket: GLAUKO.005C1

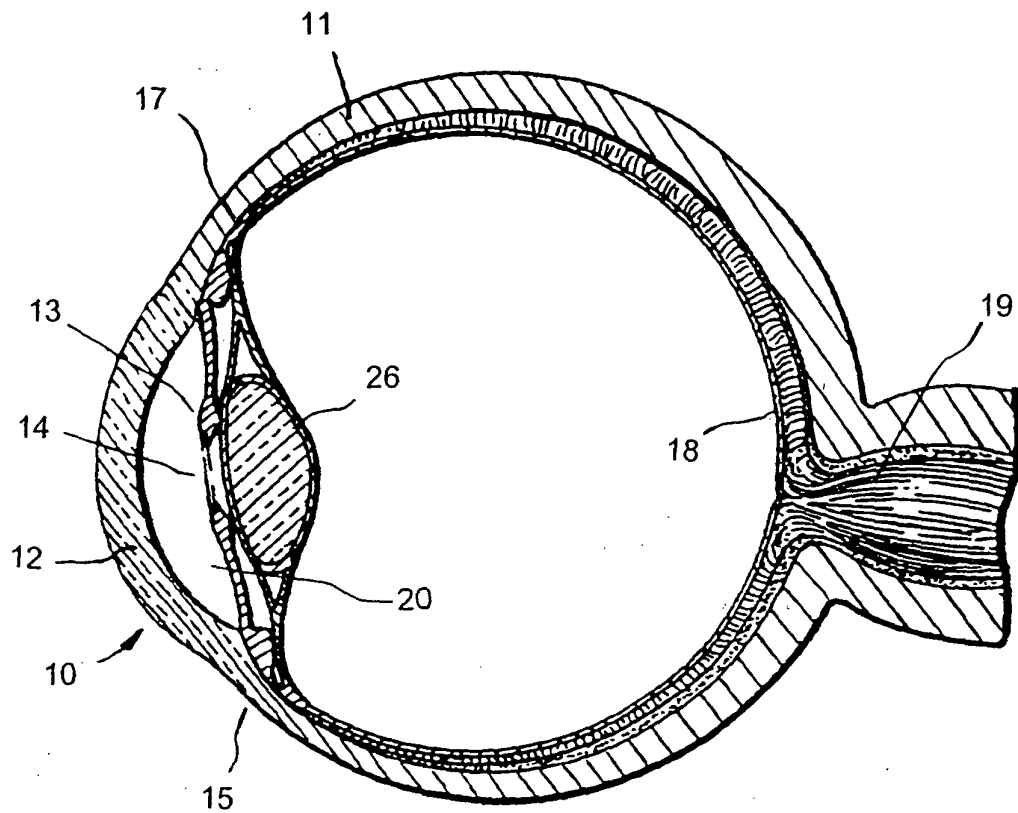


FIG. 1



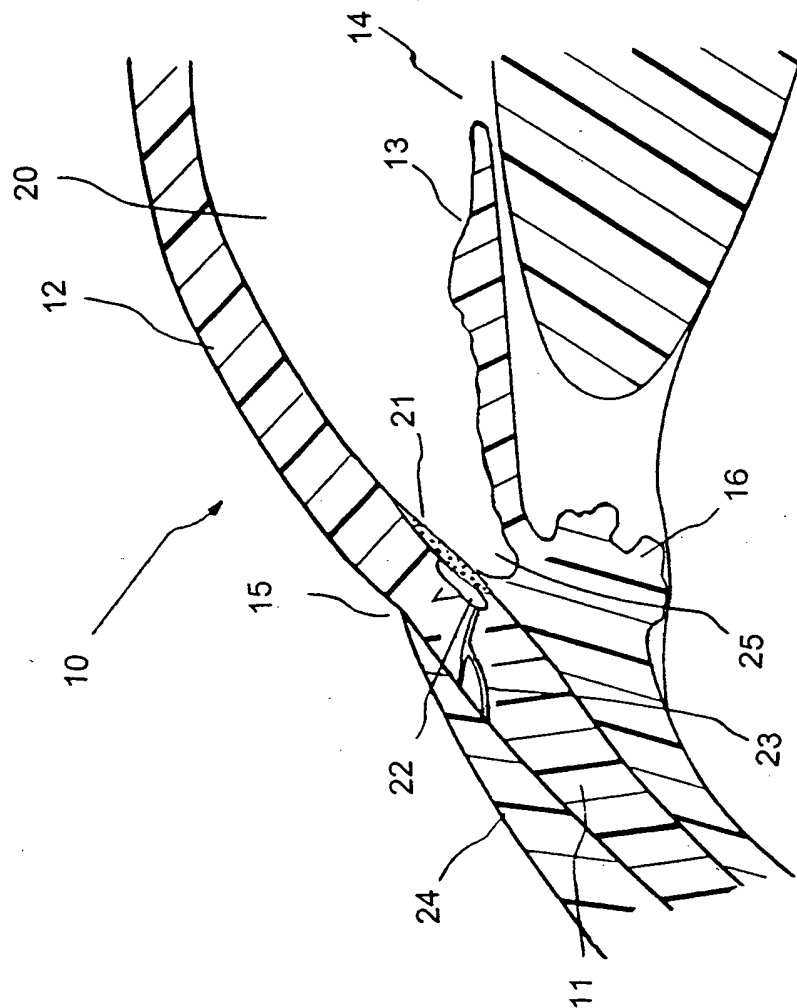


FIG. 2

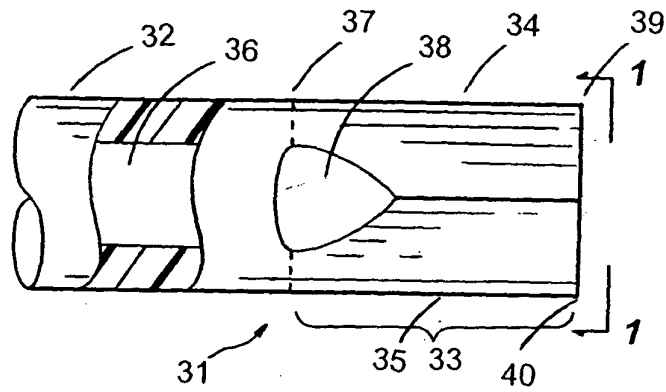

**FIG. 3A**



**FIG. 3B**

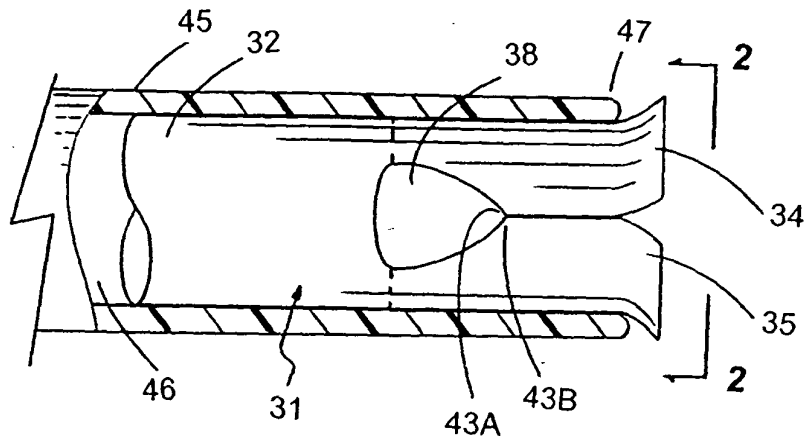


FIG. 4A




FIG. 4B



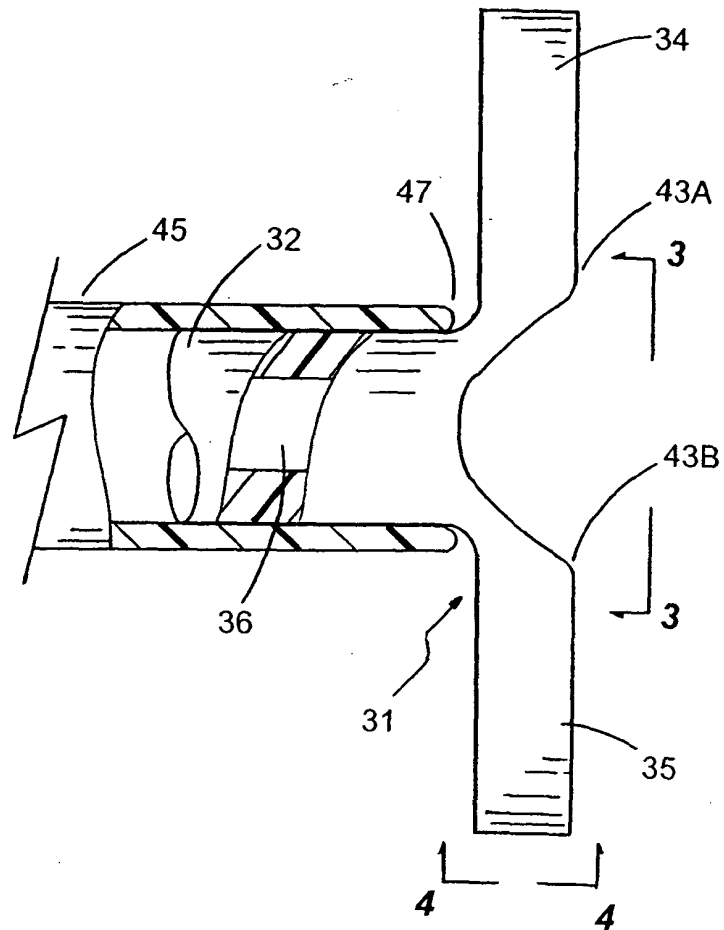


FIG. 5A

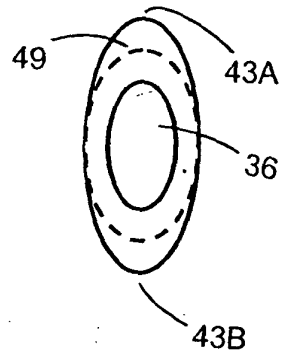

**FIG. 5B**



**FIG. 5C**

IMPLANT WITH PRESSURE SENSOR FOR GLAUCOMA TREATMENT

Morteza Gharib, et al.

Appl. No.: Unknown

Atty Docket: GLAUKO.005CI

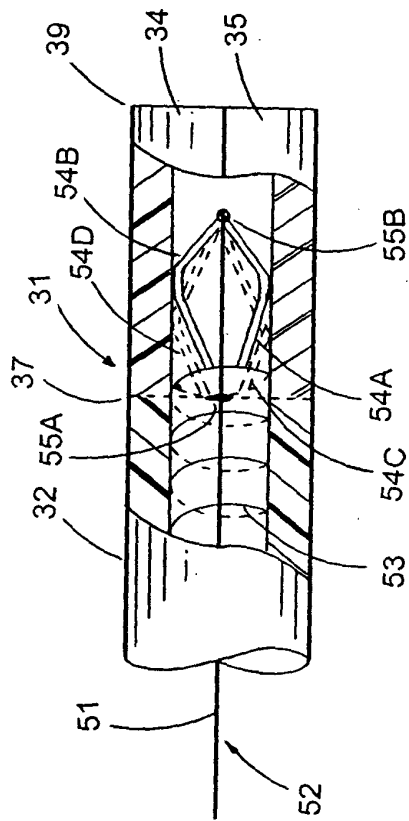


FIG. 6

IMPLANT WITH PRESSURE SENSOR FOR GLAUCOMA TREATMENT

Morteza Gharib, et al.

Appl. No.: Unknown Atty Docket: GLAUKO.005C1

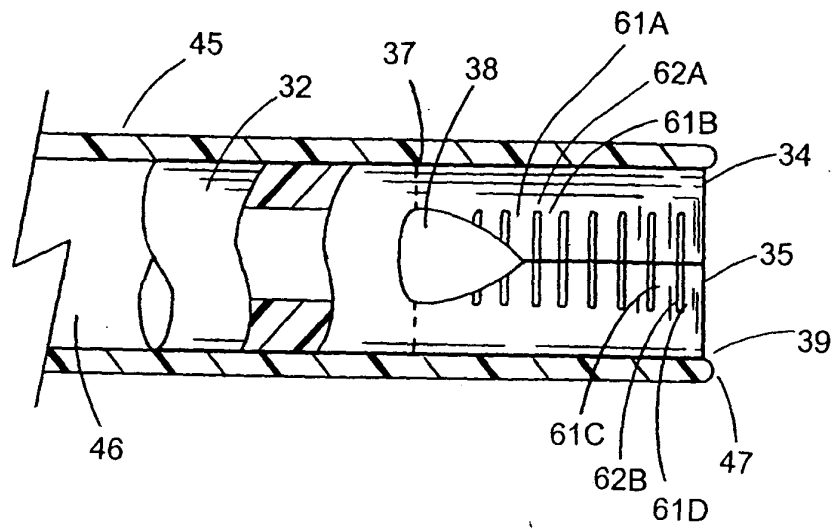



FIG. 7A



IMPLANT WITH PRESSURE SENSOR FOR GLAUCOMA TREATMENT

Morteza Gharib, et al.

Appl. No.: Unknown Atty Docket: GLAUKO.005C1

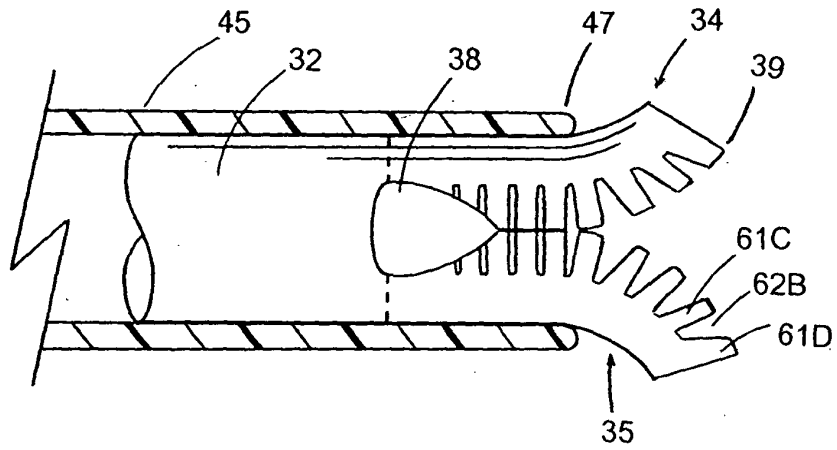

**FIG. 7B**

IMPLANT WITH PRESSURE SENSOR FOR GLAUCOMA TREATMENT

Morteza Gharib, et al.

Appl. No.: Unknown

Atty Docket: GLAUKO.005C1

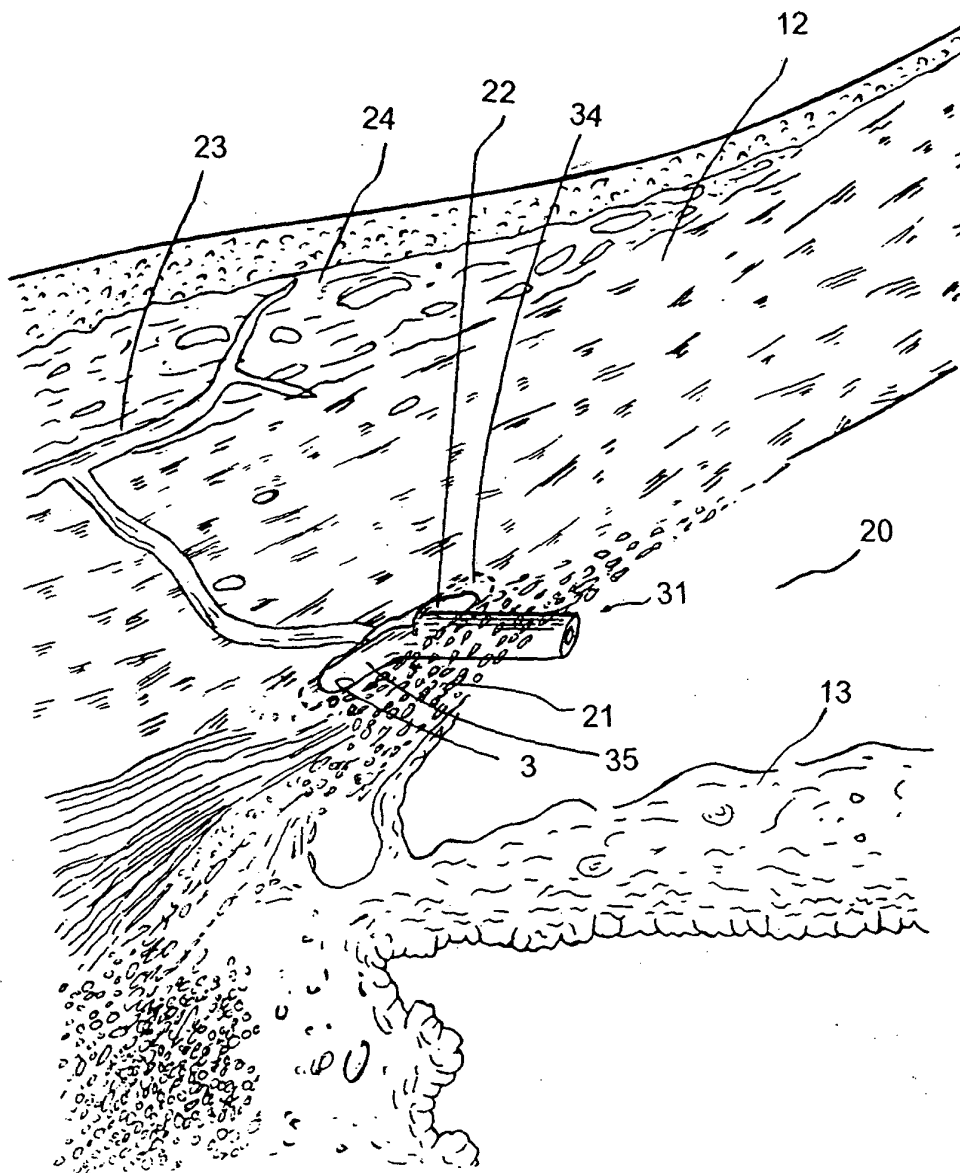


FIG. 8